


Graph 6
 Second Marker Sample
 Laboratory
 Standard Deviation of Nicotine Analysis

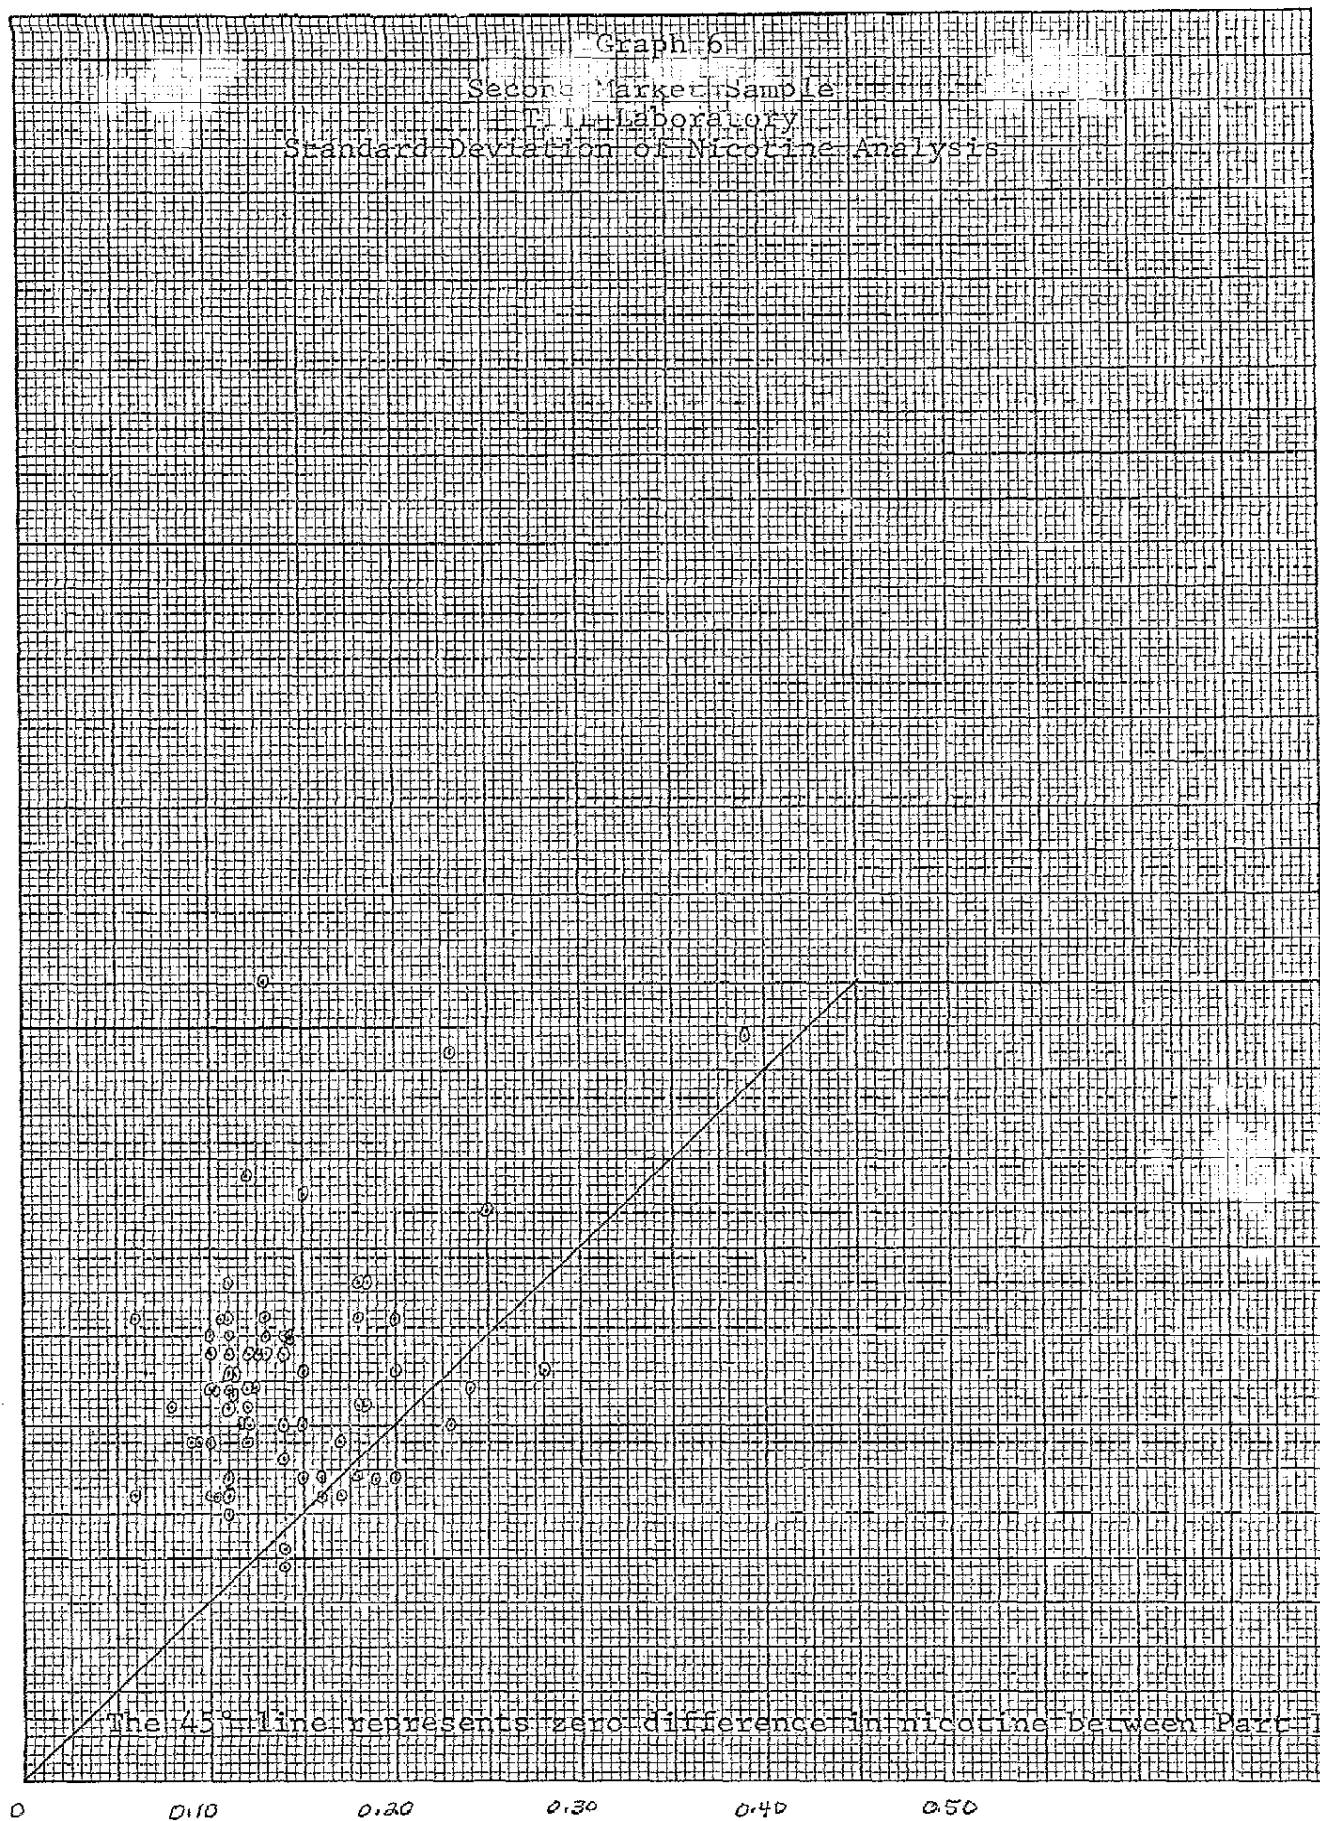

The 45° line represents zero difference in nicotine between Part I &

PART II - Standard Deviations, mg/kg

PM3001013827